

Novel approach to correlative imaging

by Dykas Michal, Correscopy

What is correlative imaging?

Increasing demand of high quality research forces research community to find new ways of data acquisition. Important part of the research is data acquired from imaging devices. Imaging using various types of microscopy or spectroscopy is an essential technique used in many types of research in both academia and industry. Imaging of a single sample (or part of it) can be performed using number of techniques subsequently and the collected data can be compared and correlated, such imaging is named a correlative imaging. The correlative imaging, or correlative microscopy, was conventionally related strictly to correlation of the information acquired from two imaging devices about exactly the same location on a sample (e.g. a single cell), usually: a Light Microscope (LM) and a Scanning Electron Microscope (SEM). To achieve such correlation manufacturers offer interchangeable sample holders or produce very sophisticated all-in-one imaging devices.

From the data obtained using correlative imaging techniques, many additional parameters of the sample can be discovered and calculated by using already available on the market image (data) correlation software - resulting in the conclusions which can be made without a doubt.

Where are the problems?

Availability of the solutions.

Imaging devices used for correlative imaging are often very sophisticated machines which require very high initial investments, on which most of the laboratories are not ready to take. This results in very limited access to the correlative imaging. Very few laboratories build their own custom made solutions which combine few imaging techniques they are interested in, but these are very rare. Also the available interchangeable sample holders require the laboratories to buy additional equipment from the same manufacturer as the

microscope the laboratory already owns, greatly limiting the choice. Moreover, these manufacturers offer only very limited choice of the techniques which can be correlated as there is no single manufacturer which is an expert in all available techniques [1, 2]. Such all-in-one imaging devices often compromise on the performance compared to the individual devices, reducing the quality of the data.

Lack of data for correlation.

Even the data correlation software is accessible to the researchers, the problem lies in the data availability for its processing.

There is a lack of commercial product which allows to localize exactly the same location of the sample on various imaging devices regardless of imaging technique and device manufacturer which would not have the described drawbacks.

Solution

An easily applicable device which could be used straightforward at various laboratories in many research fields would be a great solution to a problem.

- The device shall use the sample substrate which researcher is interested in, and it should not be imposed by the device.











Figure 1. Correscopy setup which comprises sample holders and adapters for various imaging devices supported by the software.

- The substrate must have no additional marks, hence no influence on the sample is possible.
- Device will allow to collect the data from exactly the same location on the sample, which will be then used by existing on the market software for the data analysis and correlation.

Correscopy developed a device which allows to get desired data from exactly the same location of the sample for the data correlation (**figure 1**). The example of the application is shown in **table 1** where four different techniques were used to image exactly the same cell. This set of the images provides large amount of the information which can be used to form a correct conclusion. It is worth mentioning that all these images were obtained from devices provided by various manufacturers as shown below. The user is not

limited anymore to single manufacturer devices. Almost any device available in one or collaborators laboratory can be freely used. As it can be observed the initial information about interesting sample can be obtained on simple light microscope which is often available on the work bench while doing experiment. If any interesting sample or sample's area is identified one can continue collecting higher quality images and different information from other devices, such as shown here: Raman Spectroscopy (RS) which provides information about vibrational, rotational, and other low-frequency modes in an observed system; Atomic Force Microscope (AFM) which provides atomic resolution image of the surface, mechanical, electrical, magnetic, etc. information about the sample; Scanning Electron Microscopy which provides high-resolution image of a surface e.g. cell morphology. Such unique set of the data

Table 1. Example of the imaging using the Correscopy device on biological sample. Imaging was done using 4 different techniques provided by 4 different manufacturers. HeLa cell was cultured in presence of carbon nanotubes for 24h and then imaged by various characterization techniques. Received set of the data gives information about the cell morphology (LM, AFM and SEM), the distribution of the CNTs inside the cell (RS) and mechanical property if the cell (AFM). Scale bar 5 μm .

Technique used	Results	Device manufacturer
Light microscopy		 Carl Zeiss
Raman spectroscopy		 Horiba
Atomic force microscopy		 Bruker
Scanning electron microscopy		 Carl Zeiss

shows great potential of the device developed by Correscopy. The other possible techniques which can be used are numerous and it mainly depends on the user's needs and access to the imaging devices. The other example, shown in **figure 2** below, presents two different sets of cells (fibroblasts) imaged by two super-resolution techniques: super-resolution LM and AFM for a direct comparison of the fluorescence data and mechanical properties of the single cell. Used imaging devices were already available at laboratory and no modifications to them were made. Cell imaging is only one example of the application of this technology, there are many other possibilities, especially in biological research e.g. histology where the same part of the tissue can be examined on each device letting no mistake to be made in the conclusion.

Biological research is only one of the possible research fields of this technology. Any field of research where imaging devices are used can greatly benefit from this technology: chemistry, material research, and engineering. Moreover, it also can be applied in commercial service imaging laboratories as the customer can exactly pin point which location of sample he is interested in and the service provider can image that particular location, creating win-win situation for both the sides. The example of the non-biological application of RS-SEM correlative image can be watched by following this link: <https://youtu.be/263fE47NHHE>

Correscopy provides the device which is customized for each set of the imaging devices

the laboratory uses. There are few minimal requirements from the device side. The device's sample stage¹ must be able to do X and Y transitions and a simple preview of a sample is required². Provided solution is ready to be used on the imaging devices, it does not require any physical modification of the device, hence guarantee won't be void or user doesn't need to obtain permission from a device owner. The wide list of microscopes and techniques, tested till now, is presented in appendix. As can be seen, for our technology it does not matter if microscope is low or high end, as well if it is old or brand new device, it works for all.

Conclusion

Correscopy provides a patented set of tools that make possible to characterize exactly the same sample on any microscope or spectroscope even if it was not prepared for it by its manufacturer. The obtained data can be easily compared and correlated using any data analysis software. The solution provides undisputed data which makes clear-cut conclusions.

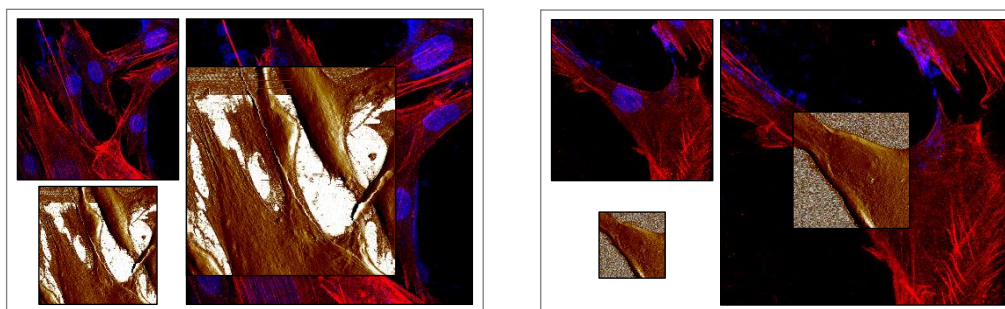


Figure 2. Fibroblasts imaged by 2 super-resolution techniques: LM (Carl Zeiss LSM 880 with Airyscan) and AFM (Bruker catalyst). The fluorescence data about the cell structure is compared directly with the AFM results which provide the information about the mechanical properties of living cell. Direct correlation of cell structure and cell mechanical property was easily obtained. FOV for LM is 140µm and for AFM images 100 µm (left image) and 60 µm (right image).

¹ Microscope stage can be provided on customer request.

² Please contact Correscopy if you need verification

About the author

Michal Dykas is a founder of Correscopy, the inventor of the solution presented in the article. He obtained Phd in integrative sciences and engineering with 5 years of experience in imaging using various techniques used in biological research, moreover he has engineering degree in automation and robotics which allows him to design tailored solutions to the imaging challenges.

About Correscopy

Correscopy is a start-up company solving real life problems regarded to correlative imaging. Correscopy provides the missing link in the imaging process which allows the direct comparison of the results obtained from various devices. Correscopy's mission is to improve quality of research by providing technology allowing direct correlation of the data.

Acknowledgements

Many thanks to the team at National University of Singapore in Singapore, Prof. T. Venkatesan from Nanoscience and Nanotechnology Institute (NUSNNI) and Prof. Yan Jie from Mechnobiology Institute (MBI) for the access to the imaging devices. Kingshuk Poddar for sample preparation, Dr. Surajit Saha and Dr. Rickson S. Winardhi for performing the imaging. Great thanks to the research team at Jagiellonian University in Cracow, Poland, for sample preparation and performing the imaging: Dr Michal Sarna and Dr Grzegorz Tylko.

References

1. Combination of high-resolution AFM with super-resolution Stochastic Optical Reconstruction Microscopy (STORM), JPK Technical note www.jpk.com/index.download.91fdb5d8cofd22156b3c9c0688127583
2. Correlative microscopy by Zeiss: http://www.zeiss.com/microscopy/en_de/products/correlative-microscopy.html

List of tested techniques and microscopes:

Technique	Microscope	Used in single experiment
Light microscopy	<i>Zeiss Primo Star</i>	
Fluorescent / Confocal Microscopy	<i>Olympus IX 81</i>	
	<i>Zeiss LSM 880</i>	
	<i>Leica DM 6000 CS</i>	
	<i>Zeiss Axiovert</i>	
Scanning Electron Microscopy	<i>Zeiss Merlin</i>	
	<i>JEOL JSM 5410</i>	
Infrared Spectroscopy	<i>Bruker Hyperion</i>	
	<i>Thermo Scientific Nicolet</i>	
Raman Spectroscopy	<i>Renishaw</i>	
	<i>Horiba HR</i>	
Atomic Force Microscopy	<i>Bruker Catalyst</i>	
	<i>Bruker Fastscan</i>	
	<i>Asylum Research MFP 3D BIO</i>	
Correlative microscopy	<i>Witec Alpha</i>	